

Laser Safety

Safe clinical application
of laser radiation

Frits F.M. de Mul

2016
www.demul.net/frits
email: ffmdemul(at)gmail.com

Laser Safety

Safe clinical application of laser radiation

Contents:

1. Physical / mathematical explanation of the calculation
2. The computer program: example of calculations.
Program options (similar calculations):
 1. Subprogram of the "Hygirad"-package (stand-alone).
 2. Web-application.

More information and downloads:

www.demul.net/frits ; "Available software....."

“Laser Safety” uses”:

NOHD: Nominal Ocular Hazard Distance


- NOHD: safe distance to avoid eye (or skin) damage
- Standard distance for eye safety:
0.25 m
for **10 s** exposure time.
- If laser intensity [W/m²] at the standard distance is too high:
protection glasses compulsory.

Damage of excessive laser exposure to eye and skin



	eye			skin	
Wave-length	Photo-chemical	Retina	Thermal	Erythema formation	Thermal
< 400 nm	+	-	+	+	+
400-600	+	+	+	-	+
600-700	-	+	+	-	+
> 700	-	-	+	-	+

NOHD: Nominal Ocular Hazard Distance

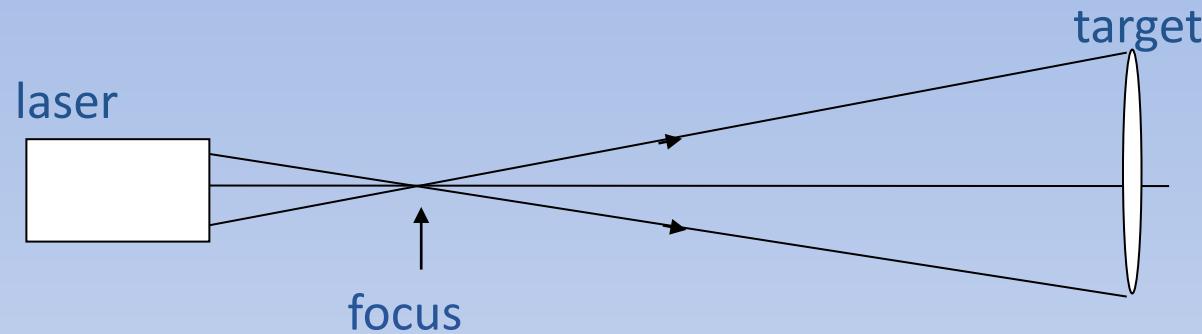

Safety condition at target:

Intensity **I** **MUST** be \leq Maximum Permissible Exposure **MPE**

I and **MPE** in W/m^2

MPE is tabulated by EU

$NOHD$ is minimum distance where **$I \leq MPE$**

MPE: maximum permissible exposure


MPE is a function of:

- Wavelength
- Pulse duration (or continuous)
- Pulse frequency
- Angular subtense (viewing angle of light source from target)


MPE-formulae are tabulated in

- Directive 2006/25/EU of European Parliament and Commission
- IEC 60825-1
- NEN 60825-1

MPE: maximum permissible exposure : eye

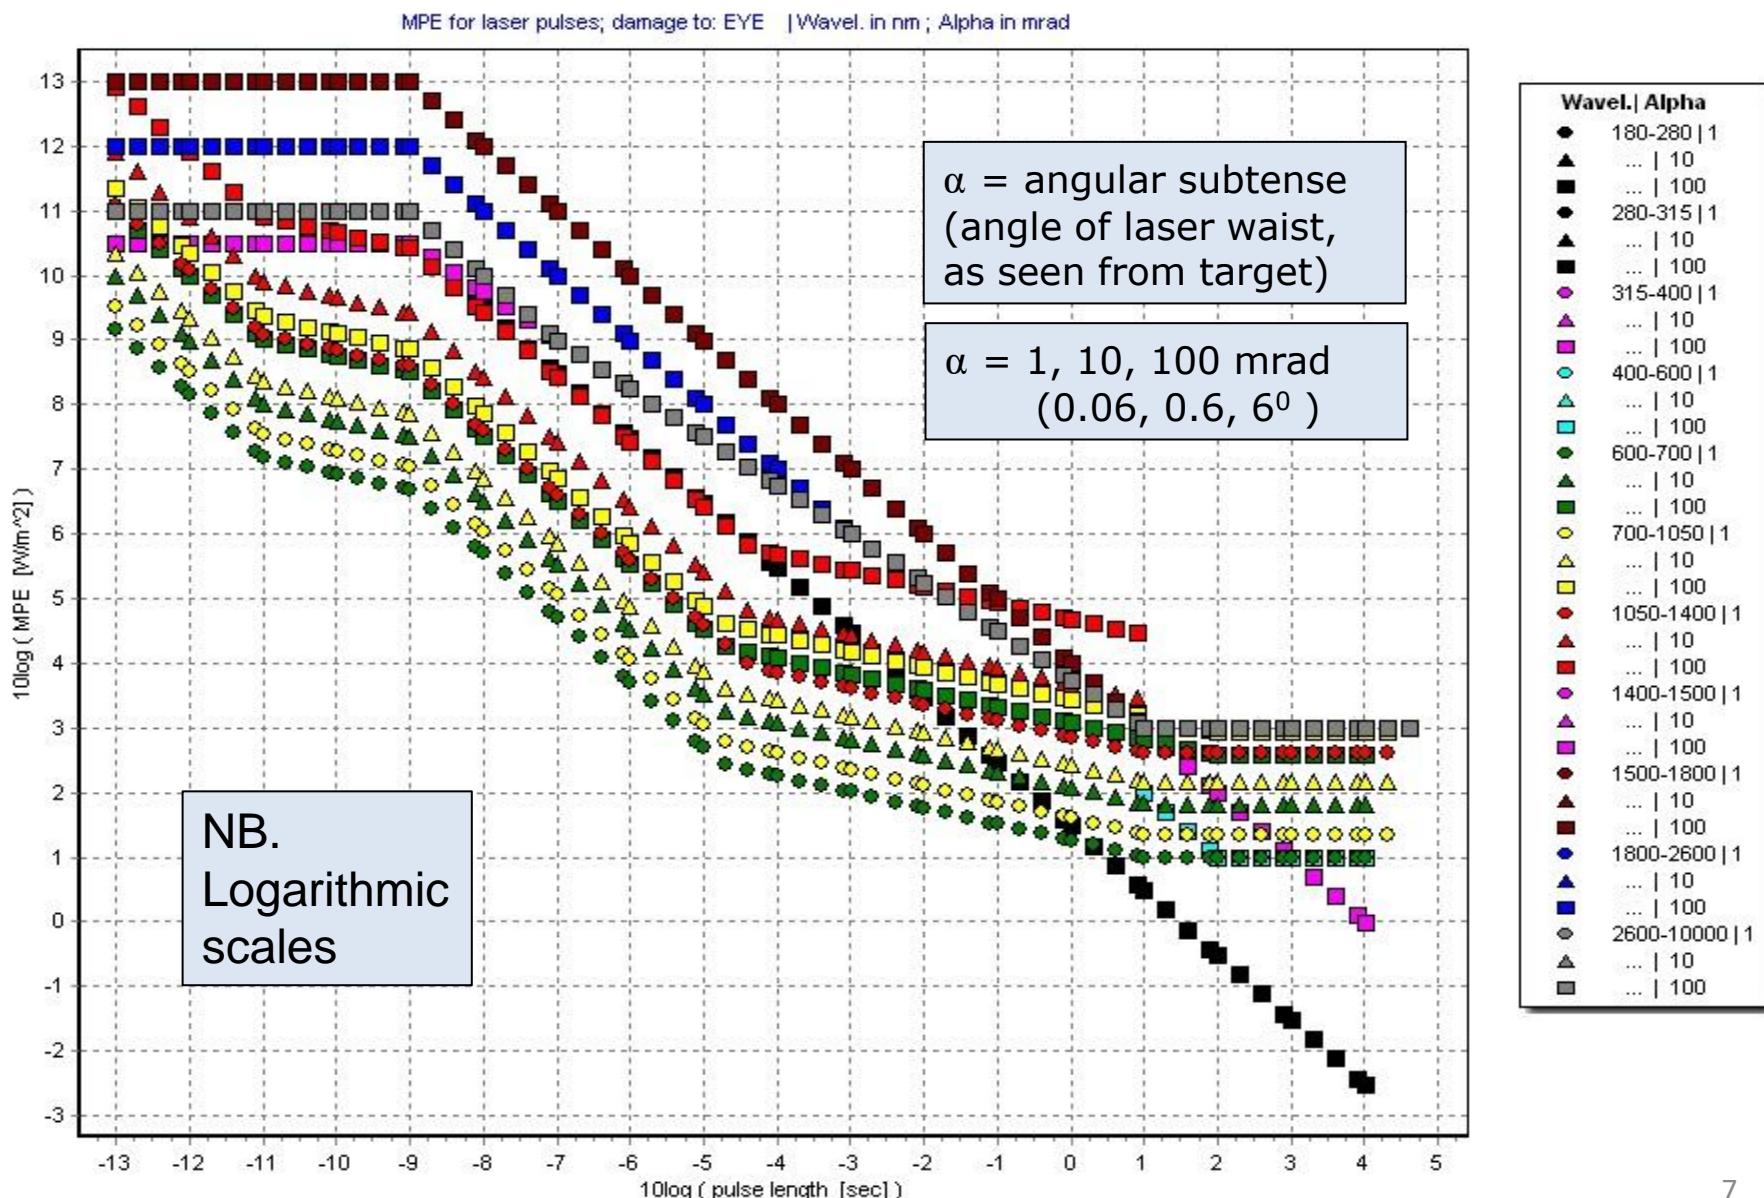

MPE: maximum permissible exposure : eye

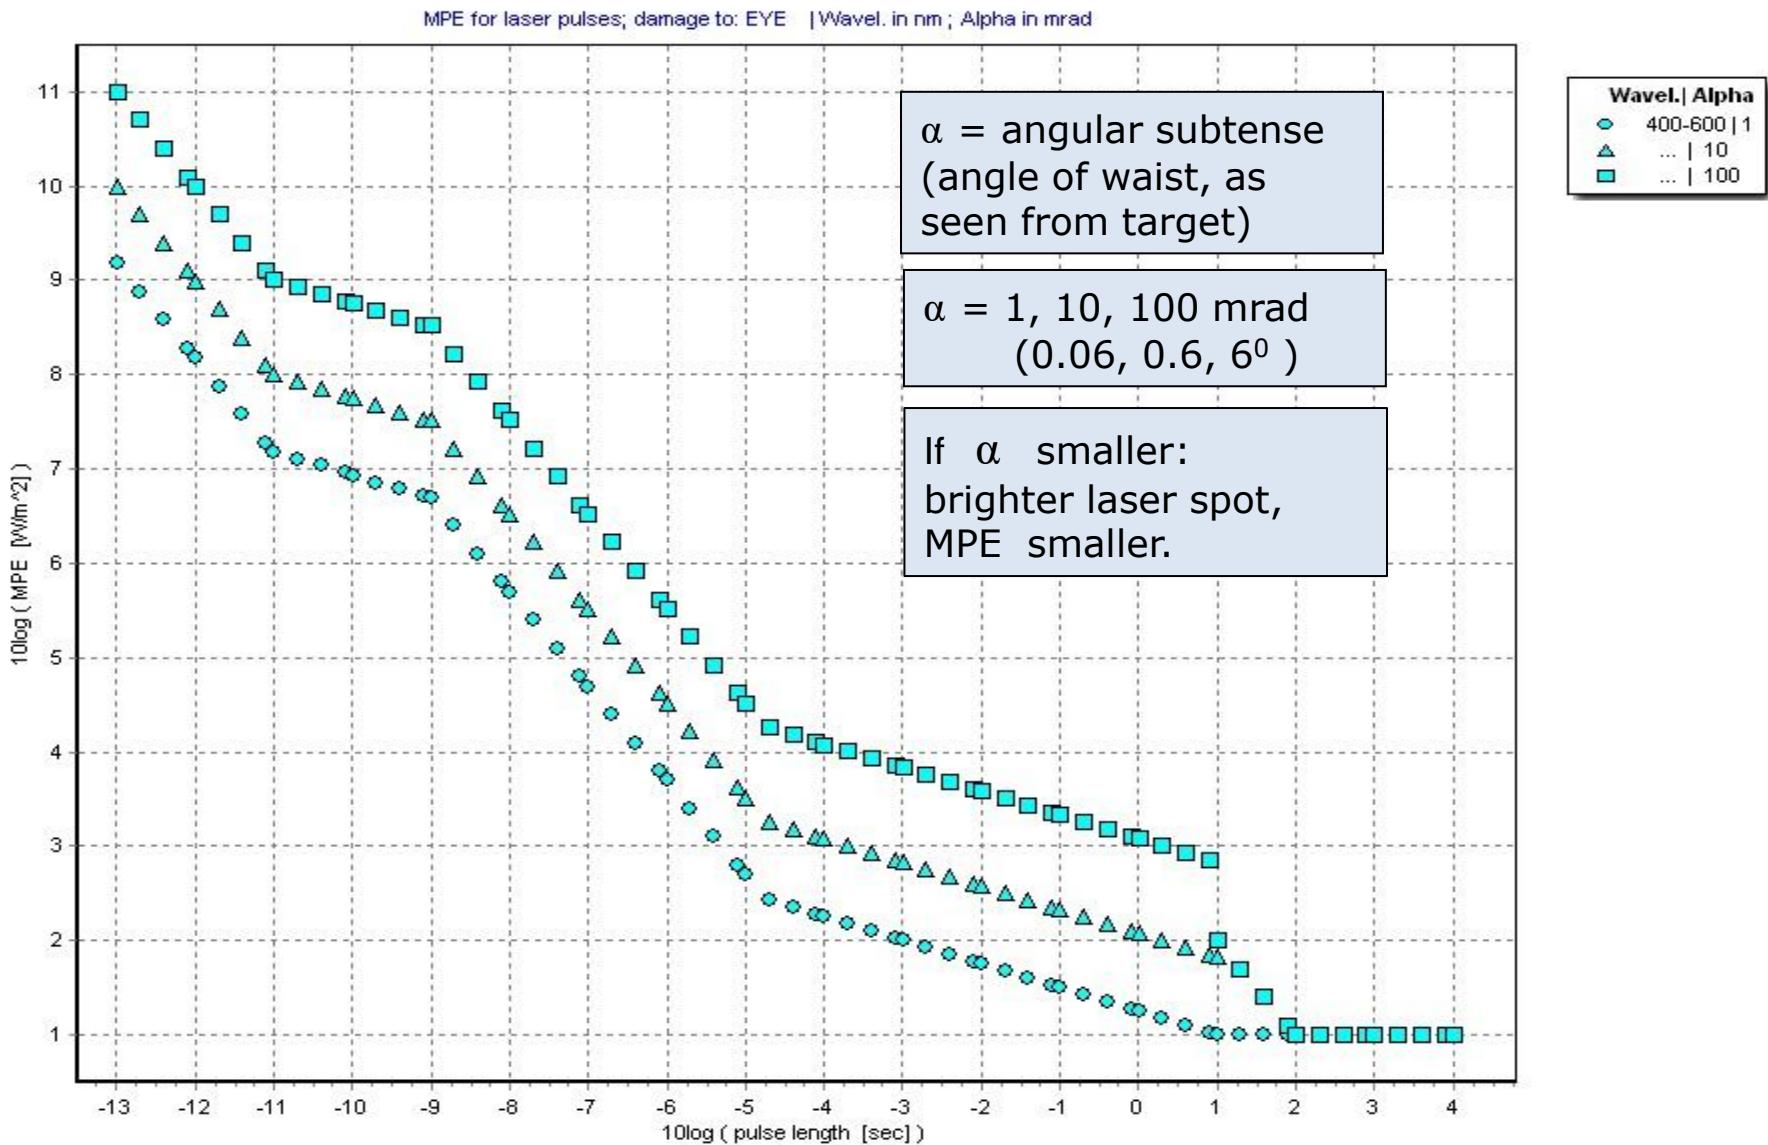


NOHD: Nominal Ocular Hazard Distance: Calculation


- Safety condition: $I \leq MPE$ in W/m²
- I = intensity [W/m²]
- $I \sim$ laser power P [W]
- $I \sim 1/\text{target area } S$ [m²]
- I dependent on type of laser beam:
 PC = laser Profile Correlation Factor [-]
- $I = (P/S) \cdot PC = P \cdot PC / S$

PC: Profile Correlation Factor

PC depends on laser mode structure

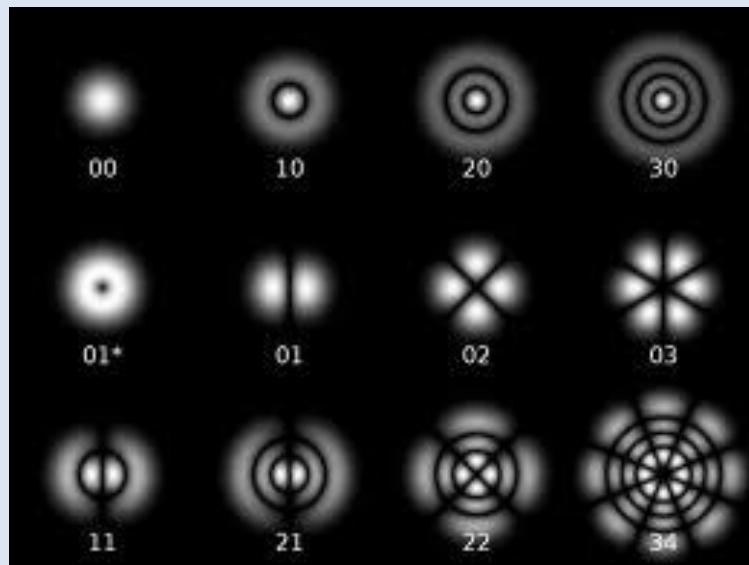

Cylindrical transverse modes

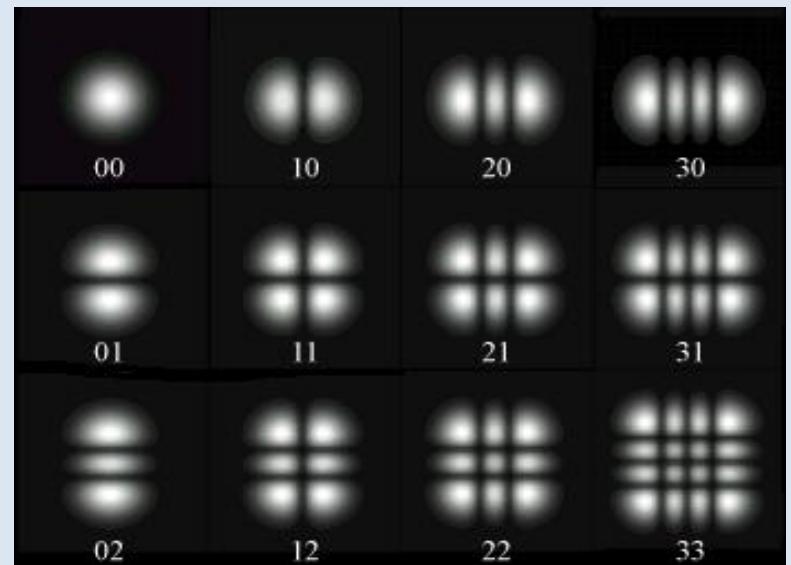

Rectangular transverse modes

Local intensity in modes is larger than averaged over the mode envelope.
→ Profile Correlation Factor **PC** > 1.

NOHD: Nominal Ocular Hazard Distance

Safety condition:

I = intensity at target

P = power

PC = prof.corr.factor

S = target area.


$$I = \frac{P \cdot PC}{S} \leq MPE \quad \Rightarrow \quad S \geq \frac{P \cdot PC}{MPE}$$

Effective target area: $S = \frac{\pi}{4} D'^2, \quad D' = D + w$

D' = effective diameter

$$S = \frac{\pi}{4} (D + w)^2$$


$$\frac{4S}{\pi} = (D + w)^2$$

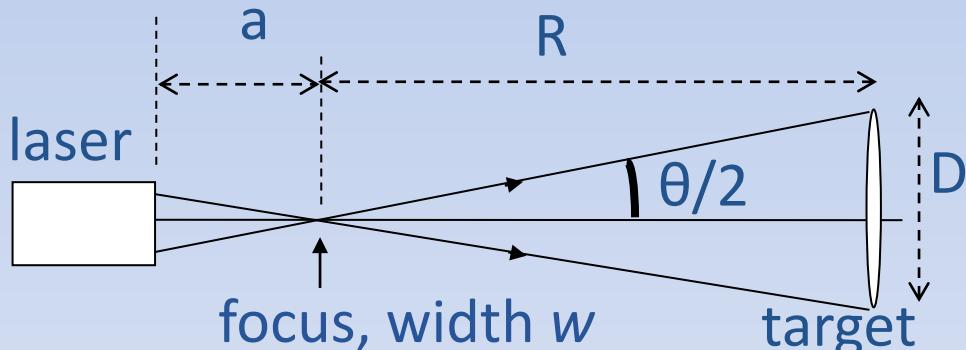

Safety condition
for target diameter :

$$D = \sqrt{\frac{4S}{\pi}} - w \geq \sqrt{\frac{4P \cdot PC}{\pi \cdot MPE}} - w$$

NOHD: Nominal Ocular Hazard Distance

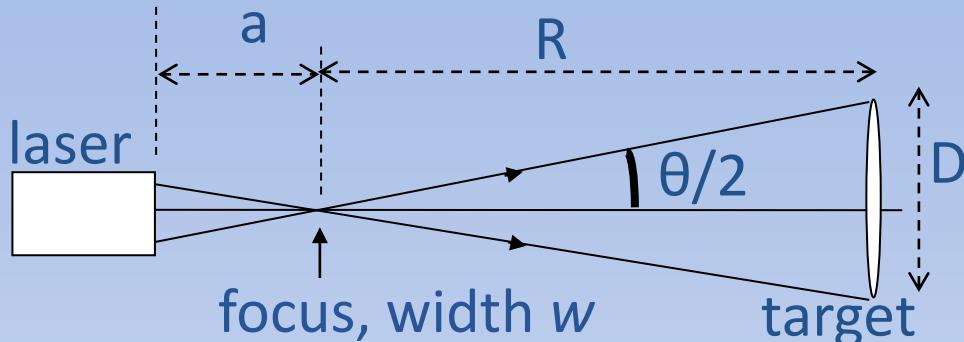

Effective target area:

$$S = \frac{\pi}{4} D'^2, \quad D' = D + w$$


Safety condition
for target diameter :

$$D \geq \sqrt{\frac{4S}{\pi}} - w = \sqrt{\frac{4P \cdot PC}{\pi \cdot MPE}} - w$$

$$NOHD = R + a = \frac{D}{2 \cdot \tan(\theta/2)} + a$$

$$NOHD = \frac{1}{2 \cdot \tan(\theta/2)} \left[\sqrt{\frac{4P \cdot PC}{\pi \cdot MPE}} - w \right] + a$$

NOHD: Nominal Ocular Hazard Distance

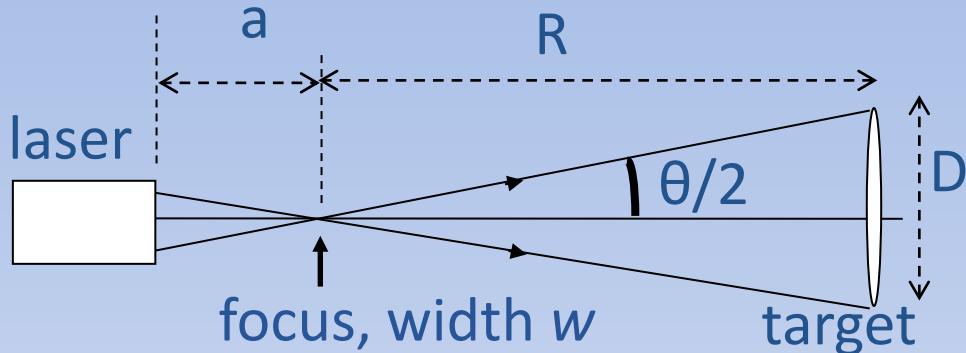

NOHD depends on:


- D , or θ
- \sqrt{P}
- \sqrt{PC}
- $\sqrt{1/MPE}$
- w
- a

$$NOHD = \frac{1}{2 \cdot \tan(\theta/2)} \left[\sqrt{\frac{4P \cdot PC}{\pi \cdot MPE}} - w \right] + a$$

NOHD: Nominal Ocular Hazard Distance

NOHD is also dependent on α : “angular subtense”

“angular subtense” α = angle to view the source (= laser focus) from the target position

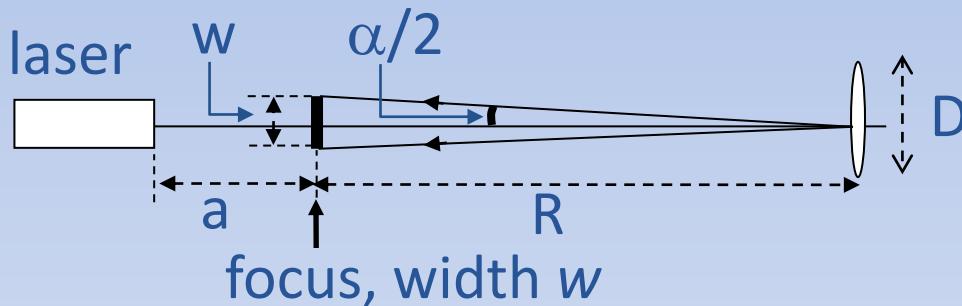

Focus as seen
from the target

$$\tan \frac{1}{2}\alpha = \frac{\frac{1}{2}w}{R} = \frac{w}{2(NOHD - a)}$$


A smaller waist will lead to a sharper (intenser) spot on the target, thus *MPE* lower.

For certain situations (e.g. visible light):

MPE depends on α (tabulated in EU-Directive),
and thus on *NOHD*


NOHD: Nominal Ocular Hazard Distance

Two relations between *NOHD* and *MPE* :

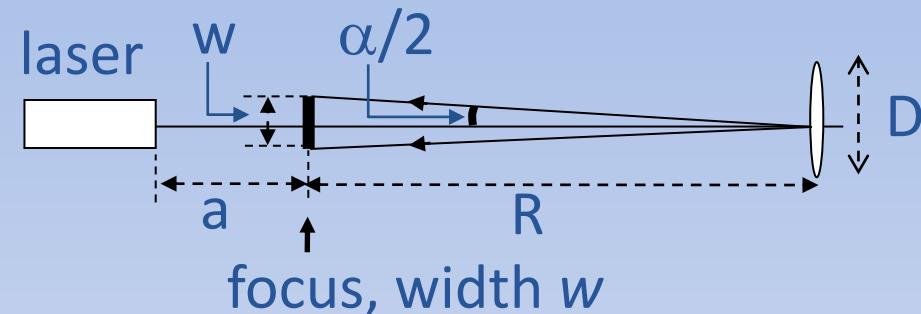

$$\tan \frac{1}{2} \alpha = \frac{w}{2R} = \frac{w}{2(NOHD - a)}$$

$$\text{So, } NOHD = f(\alpha)$$

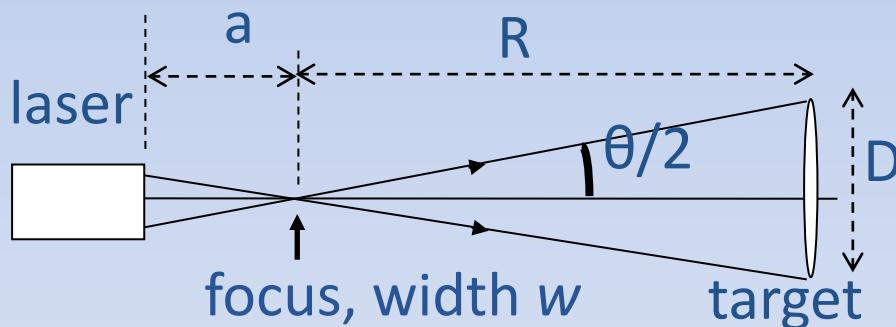

But also:

$$NOHD = f(MPE) = f(\alpha) !$$


from Safety Condition: $I \leq MPE$

$$NOHD = R + a = \frac{1}{2 \cdot \tan(\theta/2)} \left[\sqrt{\frac{4P \cdot PC}{\pi \cdot MPE}} - w \right] + a$$


Thus: iterative approach necessary !!

NOHD: Nominal Ocular Hazard Distance

Two relations between *NOHD* and *MPE* :

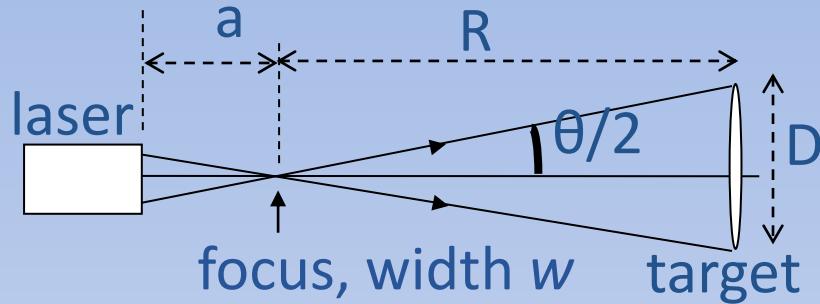


$$(1): NOHD = f(MPE) = f(\alpha)$$

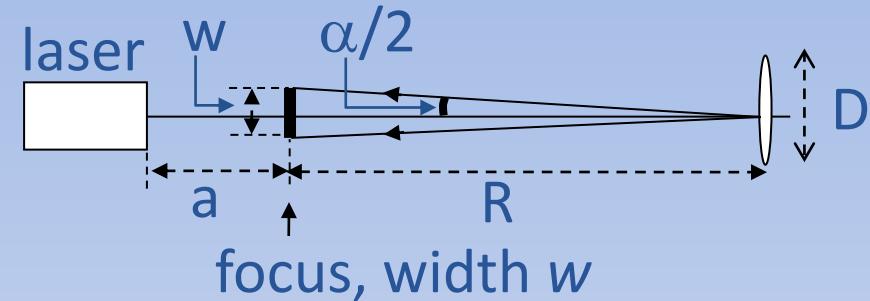


$$(2): NOHD = f(\alpha)$$

Iterative approach:

ε = tolerance

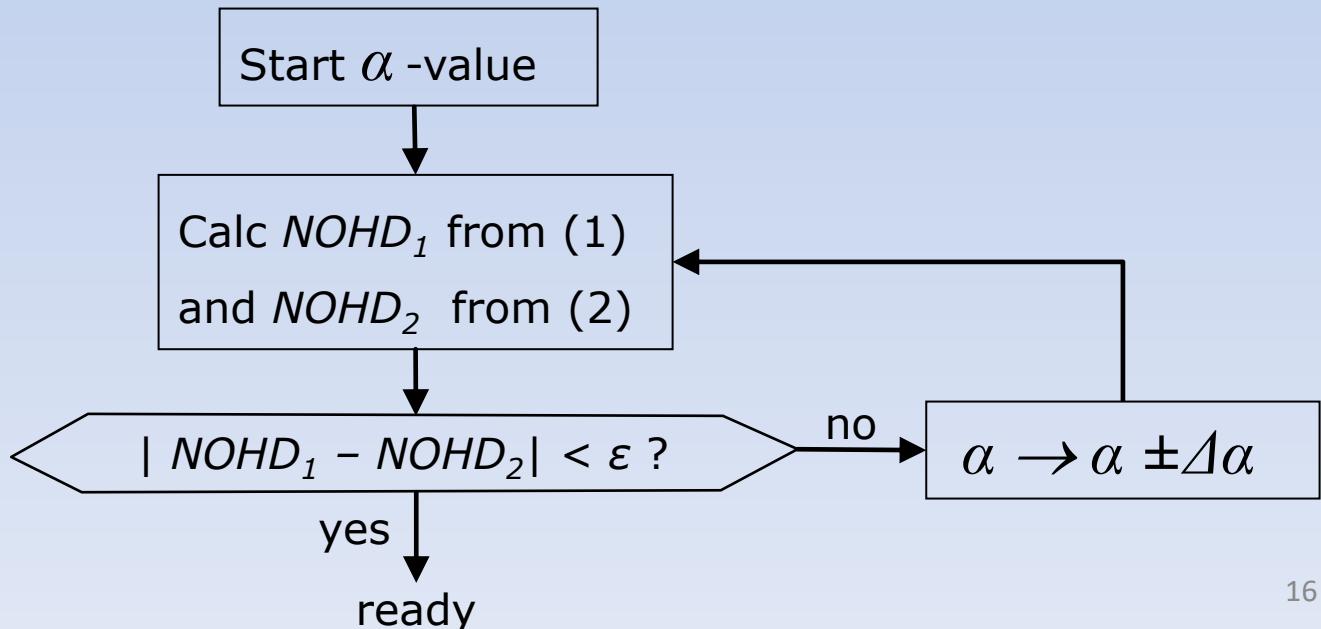

Transmission of safety goggles

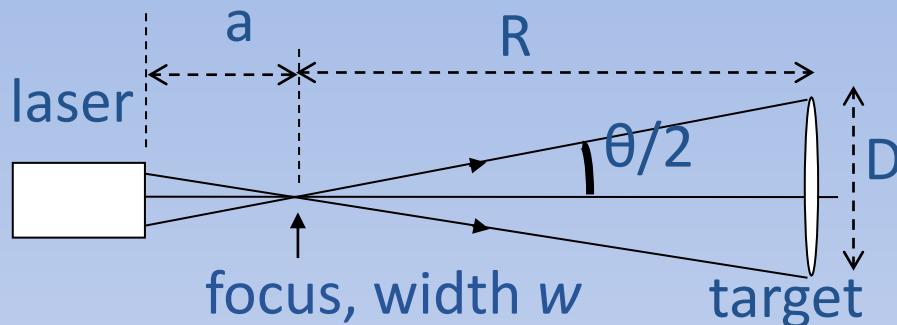

$$NOHD = R + a$$

In case $NOHD >$ safety distance b (from focus):
safety goggles necessary!

Transmission T of safety goggles and Optical density OD :


$$T = \left[\frac{b}{NOHD - a} \right]^2 ; OD = -10 \log T$$

target area $\sim R^2$

Standard safety distance = 0.25 m for 10 sec exposure.

Laser treatment

In general: pulsed laser treatment will consist of
 ≥ 1 separate trains of ≥ 1 separate pulses

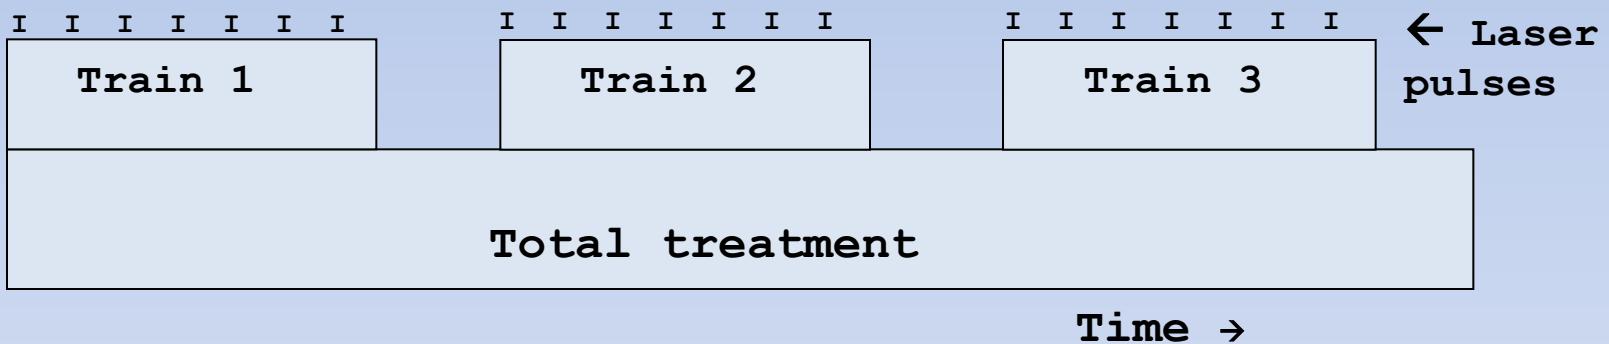

Continuous laser: 1 long train of 1 long pulse.

Hygirad-program: Example of calculations

LASER INPUT DATA	VALUE	
wavelength	532	nm
(full) Divergence angle	0.0125	rad
Profile correlation factor	2	-
Waist(spot)diameter	400e-6	m
Distance laser to focus(waist)	0.3	m
Basic pulse: pulse power	1.000E+06	w
....: pulse energy	5.000E-03	J
....: duration	5.000E-09	s
....: rep.freq.	1000	Hz
Train of pulses: power	5.000E+00	w
....: energy	5.000E+01	J
....: duration	1.000E+01	s
....: rep.freq.	0.100	Hz
....: pulse at end of train (yes/no=1/0)	0	-
....: nr. of pulses per train	10000	-
Total treatment: power	5.000E+00	w
....: energy	5.000E+01	J
....: duration	1.000E+01	s
....: nr. of trains in total	1	-
Safe distance from focus (for OD-glasses)	0.250	m

Hygirad-program: Example of calculations

OUTPUT of calculations:

For this wavelength the damage is:

EYE: photochemical and retina (thermal) and thermal
SKIN: thermal

RESULTS: (H in J/m² - E=MPE in W/m²)

CALCULATION	formula	MPE [W/m ²]	alpha [rad]	NOHD [m]	T-glasses	OD-glass
eye: pulse	H=5E-3.CE	1.000E+06	3.133E-06	127.9	3.837E-06	5.416
..id. with CF1 ..	N= 10000, CF= 1.000E-01	1.000E+05	9.906E-07	404.0	3.836E-07	6.416
..id. with CF2 ..	N= 10000, CF= 1.000E-01	1.000E+05	9.906E-07	404.0	3.836E-07	6.416
eye: train	H=18.CE.t ^{0.75}	1.012E+01	4.461E-06	89.99	7.769E-06	5.110
eye: total	H=18.CE.t ^{0.75}	1.012E+01	4.461E-06	89.99	7.769E-06	5.110
skin: pulse	H=200.CA	4.000E+10	6.605E-04	0.906	1.700E-01	0.769
..id. with CF1 ..	N= 10000, CF= 1.000E-01	4.000E+09	2.012E-04	2.286	1.584E-02	1.800
..id. with CF2 ..	N= 10000, CF= 1.000E-01	4.000E+09	2.012E-04	2.286	1.584E-02	1.800
skin: train	H=1.1E4.CA.t ^{0.25}	1.956E+03	6.230E-05	6.722	1.515E-03	2.819
skin: total	H=1.1E4.CA.t ^{0.25}	1.956E+03	6.230E-05	6.722	1.515E-03	2.819

CF = correction factor, needed for thermal damage when >1 pulse in Tmin.
(Tmin is 1.8E-5 s for 532 nm).

the end